

Air Pollution Sensors in Hamilton and how can they help?

Dr. Matthew Adams

About Me

- Professor in the Department of Geography, Geomatics and Environment at the University of Toronto Mississauga
- Research Group examines urban air pollution
 - GTHA
 - Peel / Hamilton have a greater focus
 - Africa – Rwanda
 - Brazil
- Coming to you live from Dundas



Overview

- Air Sensors
- Particulate Matter
 - Air Monitors Overview
- Our Experience with PM Sensors in Hamilton
- Best Practices
- Recommendations

Air Monitor vs. Air Sensor

Air Monitor – Defined in North America by EPA Standards (\$\$\$)

- Must meet specific performance guidelines
 - Federal Reference Methods
 - Federal Equivalent Methods

Air Sensor – Low-cost device (\$)

- No performance guidelines

Air Pollution Sensors

- Air sensors are low-cost
- Often portable devices
- Should be easily operated
 - i.e. minimal technical training

Air Sensor Use: Education

- Using sensors in educational settings for science, technology, engineering, and math lessons.



Air Sensor Use: Information /Awareness

Using sensors for informal
air quality awareness

Carnegie Mellon University

News

Stories

Media Highlights

Media R

[News](#) > [Stories](#) > [Archives](#) > [2016](#) > [March](#) > CMU, Airviz Will Make Air Quality Monitors Available at Public Libraries Nationwide

March 15, 2016

CMU, Airviz Will Make Air Quality Monitors Available at Public Libraries Nationwide

Sensor Data Gives People Power To Improve Air They Breathe



SIGN IN

NPR SHOP

DONATE

NEWS ARTS & LIFE MUSIC SHOWS & PODCASTS SEARCH

National

Politics

Health

Technology

World

ENVIRONMENT

Business

Science

Race & Culture

May 24, 2015 6:03 PM ET

Heard on All Things Considered



LARKIN PAGE-JACOBS

A Home Air Quality Monitor That Can Be Checked Out From The Library

FROM 90.5 WGBA

Air Sensor Use: Personal Monitoring

Monitoring the air quality that a single individual is exposed to while doing normal activities.



Air Sensor Use: Supplementing Monitoring Network

- Governmental monitoring is currently examining the ability to use lower cost sensors to supplement monitoring networks.



Environment International


Volume 99, February 2017, Pages 293–302



Full length article

Can commercial low-cost sensor platforms contribute to air quality monitoring and exposure estimates?

Nuria Castell ^a , Franck R. Dauge ^a, Philipp Schneider ^a, Matthias Vogt ^a, Uri Lerner ^b, Barak Fishbain ^b, David Broday ^b, Alena Bartonova ^a




Air Sensor Use: Source Identification and Characterization

Establishing possible emission sources by monitoring near the suspected source.



Particulate Matter

- Mixture of solid particles and liquid droplets found in the air
 - Not a single chemical or pollutant
- May be directly emitted into the atmosphere
- Forms by chemical reactions from combinations of other pollutants

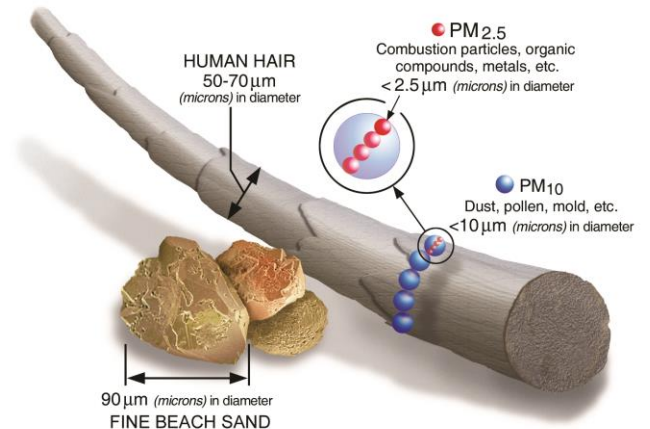

PM_{2.5} Federal Reference Method

- 24-hour samples
- Air is drawn at a constant rate into a specially shaped inlet and through a particle size separator
- Particles <2.5 microns are collected on a PTFE (Teflon) filter.



Particle Separation

Aerosol Impaction


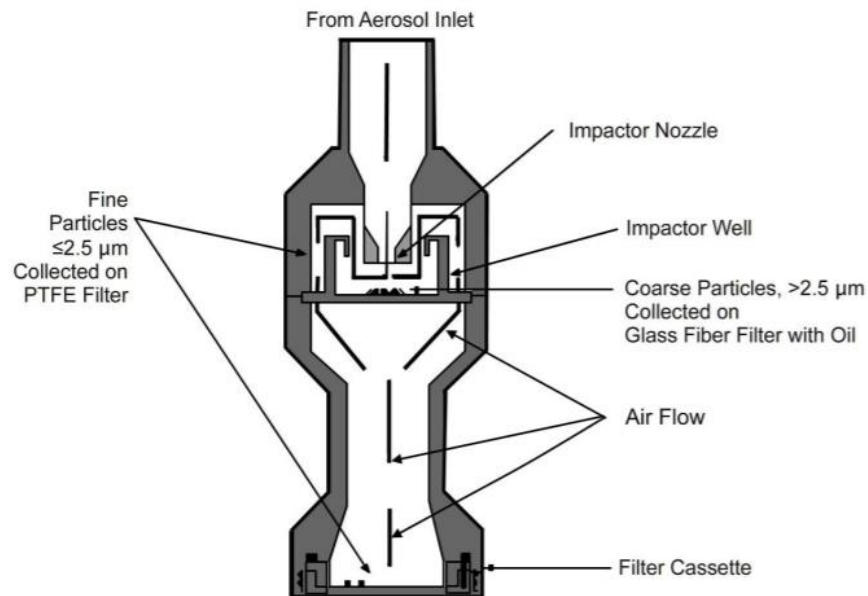


Figure 4-15. WINS particle impactor and filter holder assembly.

VSCC (Very Sharp Cut Cyclone)

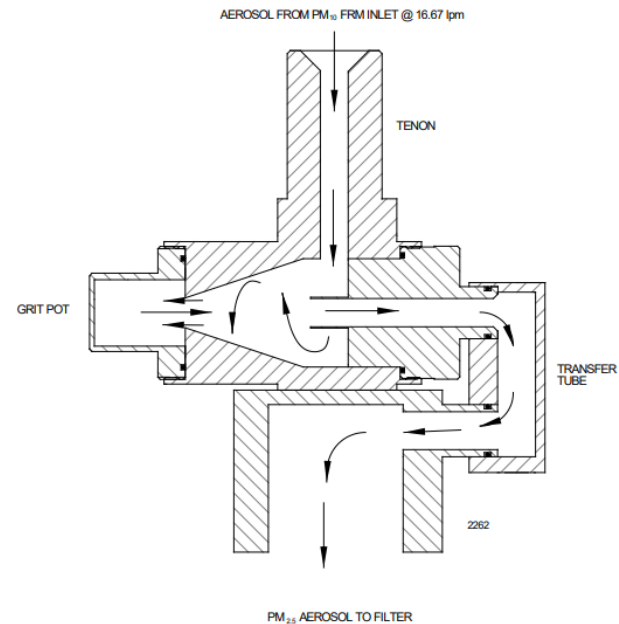

Gravimetric Analysis (PM_{2.5} FRM)

- Filters are conditioned to a constant temperature and RH.
- Prior to sampling filters are weighed
- Post sampling filters are reweighed and the difference in mass is used along with the volume of air to determine concentration



PM_{2.5} FEM Real-time monitors

- Beta Attenuation Mass Monitor
 - Particles are collected on a filter and particle mass is determined by change in beta radiation absorption
- Tapered element oscillating microbalances (TEOM)
 - Filter is oscillating by two magnets, increased mass changes oscillation rate.
- Light scattering continuous ambient particulate monitor
 - Particles flowing past a light cause scattering. The scattered light pulse is related to particle size.



Measurement Units

- Micrograms per cubic meter of air
 - $\mu\text{g}/\text{m}^3$
- Perspective
 - Dime is 1750 μg
 - Grain of salt is 300 μg
 - Eyelash is 40 μg



PurpleAir Sensor

- Laser Particle Counters
 - Two in each unit
- Particles are classified into five size bins
 - Particle mass is estimated
- Provides PM_{10} , **$PM_{2.5}$** and PM_{10} concentration data
- Connects to Wi-Fi


Performance When New

Collocation of the air sensors and an air monitor for 59 days.

Both used light scattering as the principle of operation.




Performance When New

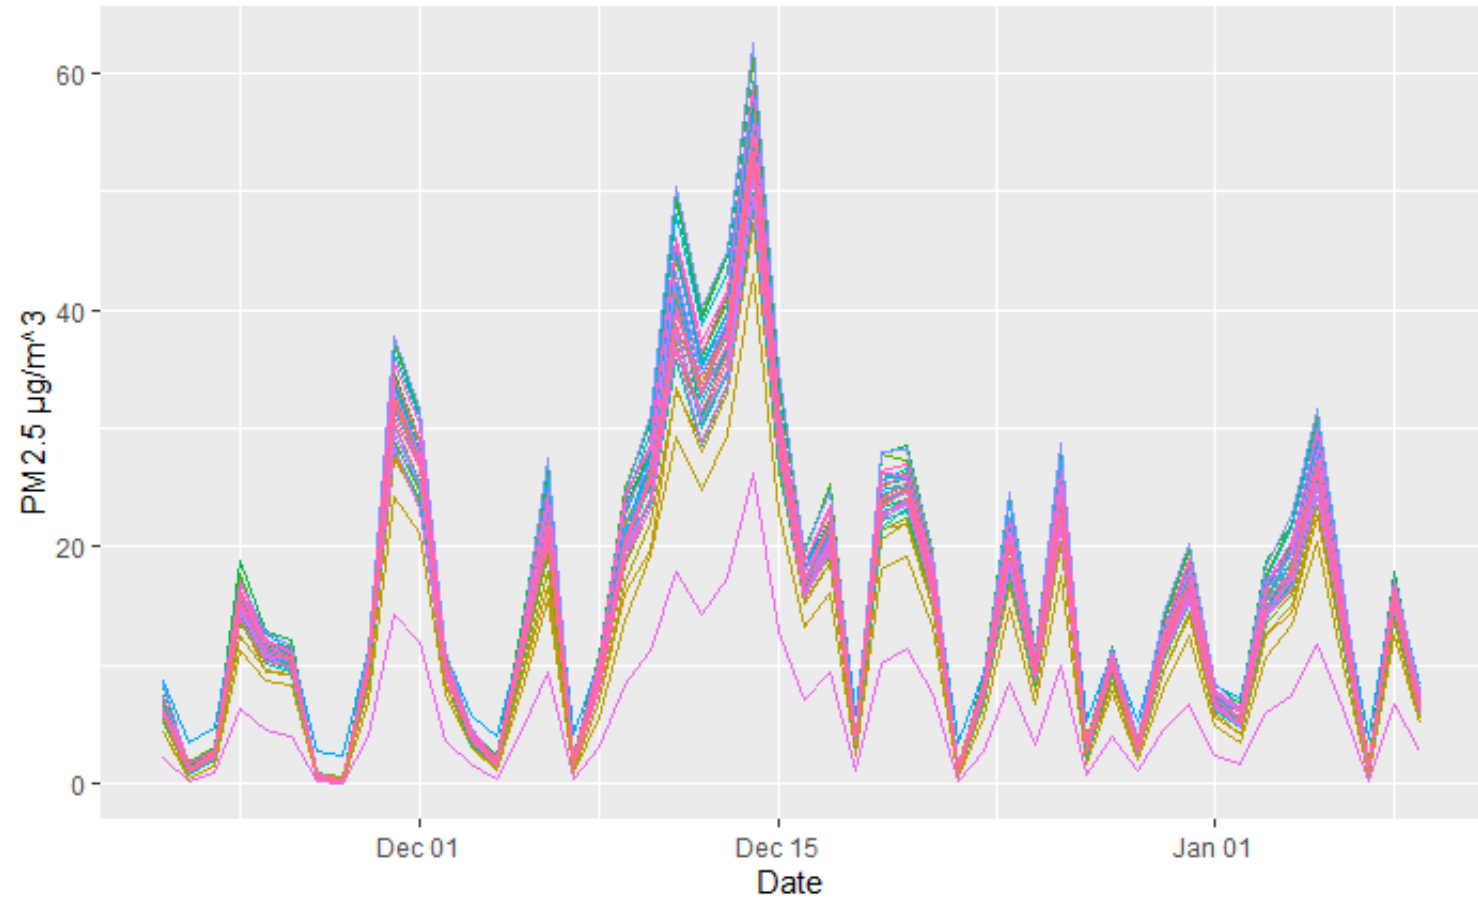


Average of Purple
Air Monitors

Reference
Monitor

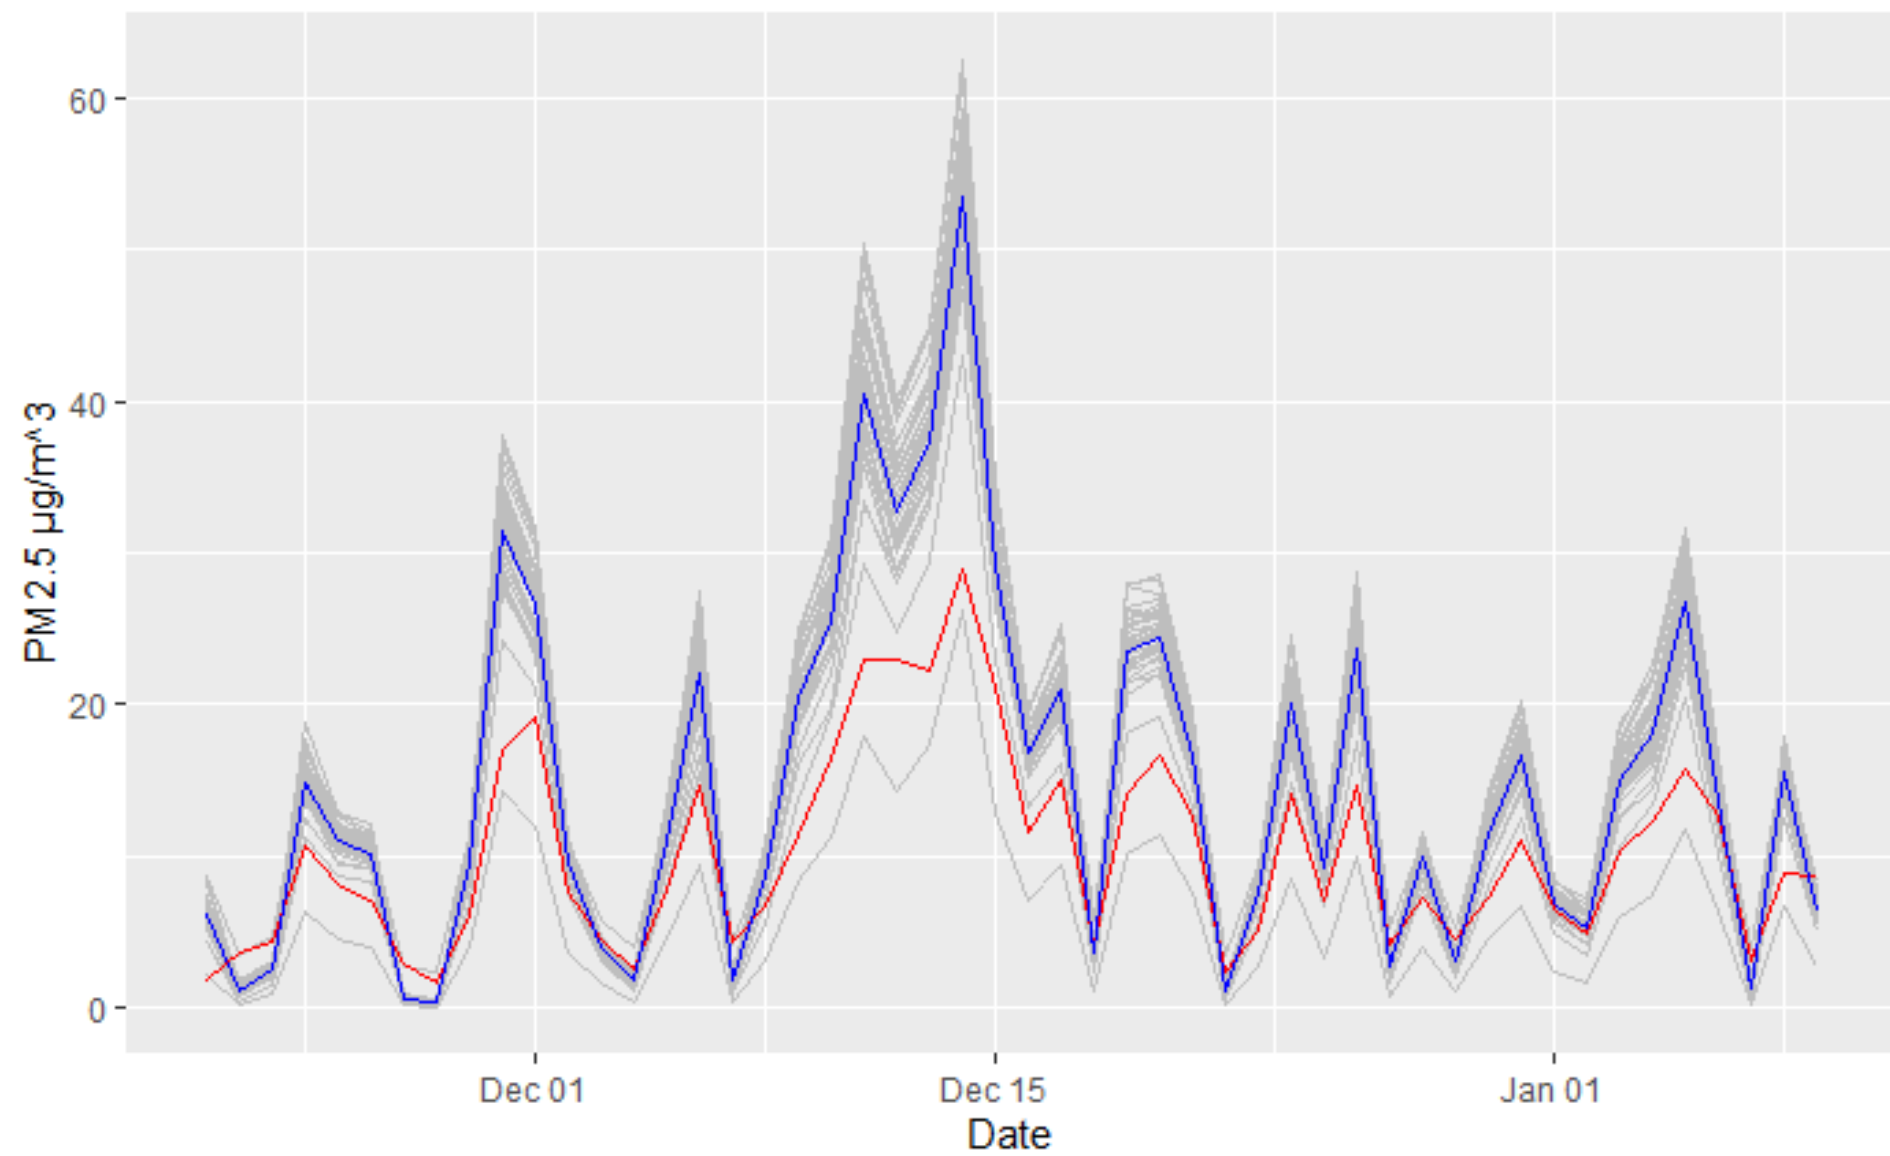

Daily Averages


- Reference Monitor
 - Range: 1.6 - 29 $\mu\text{g}/\text{m}^3$
 - Average (Mean): 10.2 $\mu\text{g}/\text{m}^3$
- Average Error for PA Sensor
 - +4.4 $\mu\text{g}/\text{m}^3$

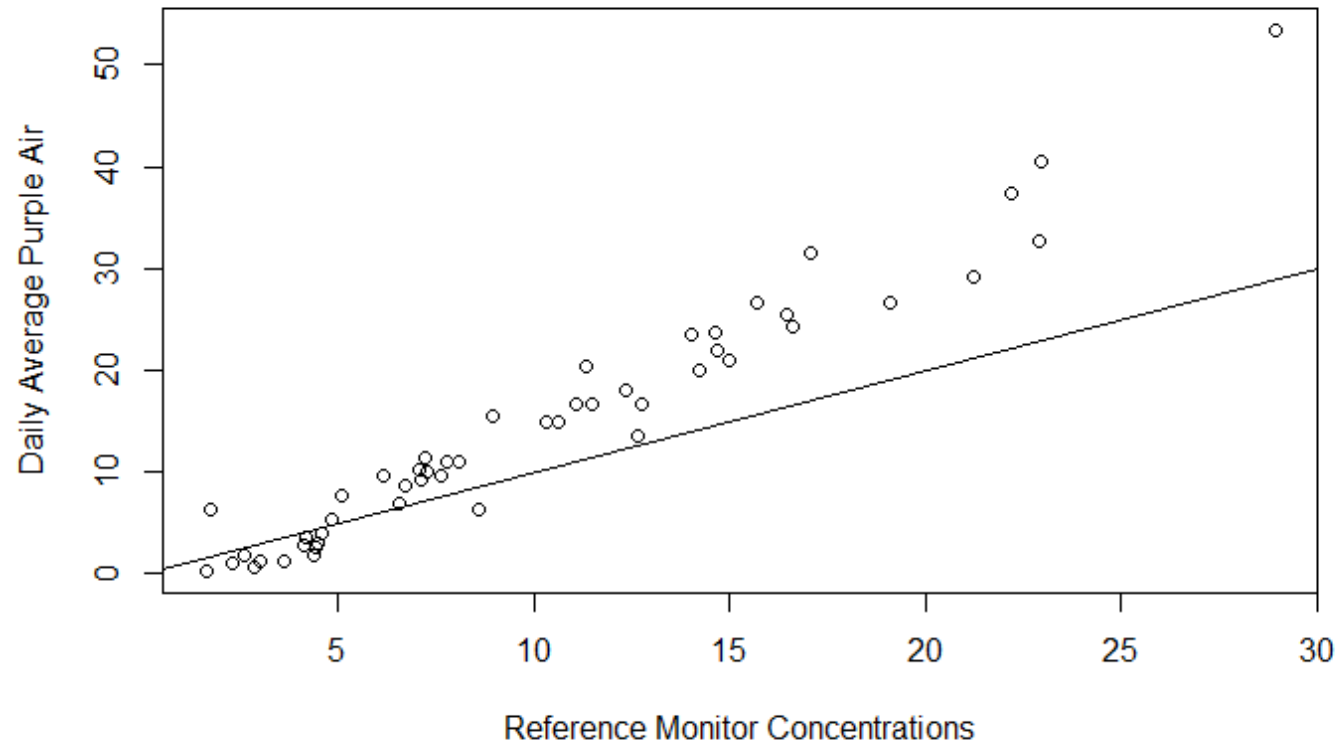


Installation

- Thanks to Environmental Hamilton!
 - We were able to identify volunteers to host air sensors.
- Distributed 35: 26 Set-up
 - Many disappeared
 - Compatibility issues


How long do they last, month(s)?

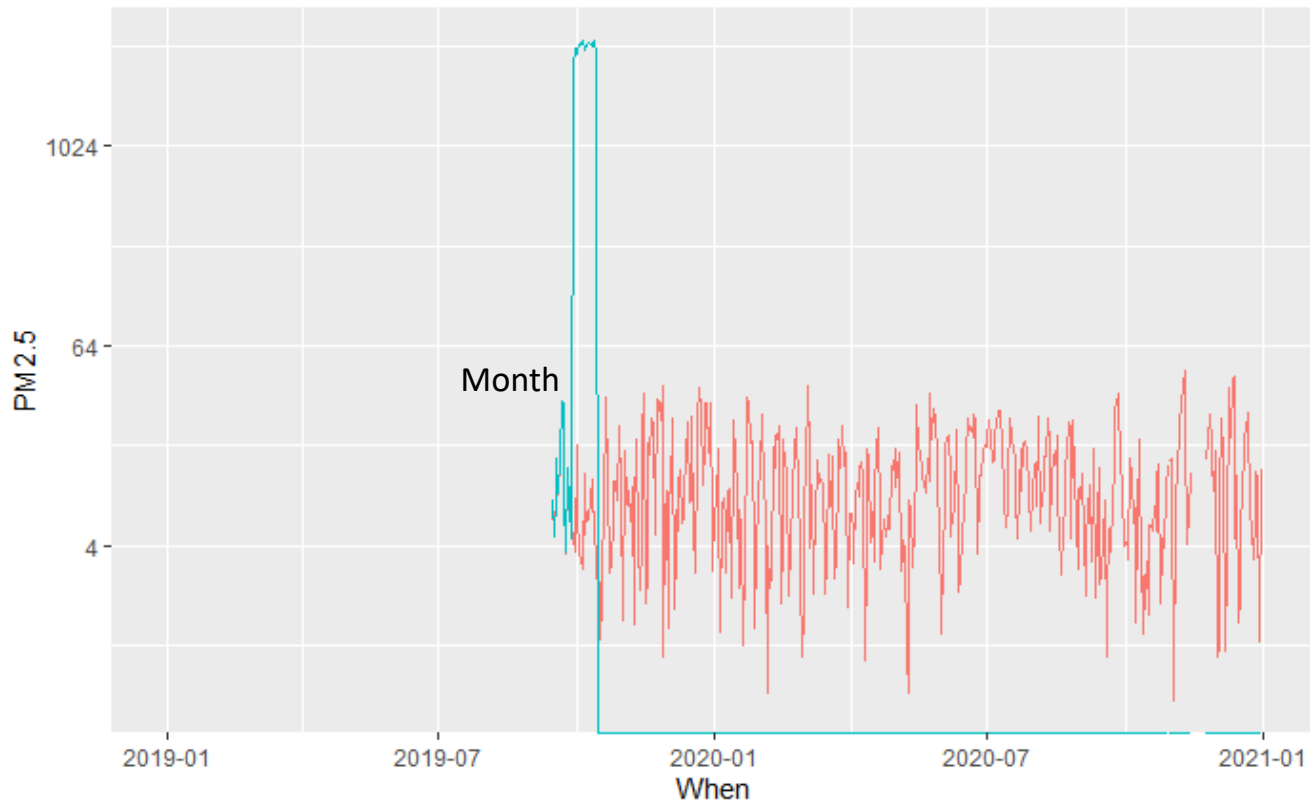


How long do they last, years?

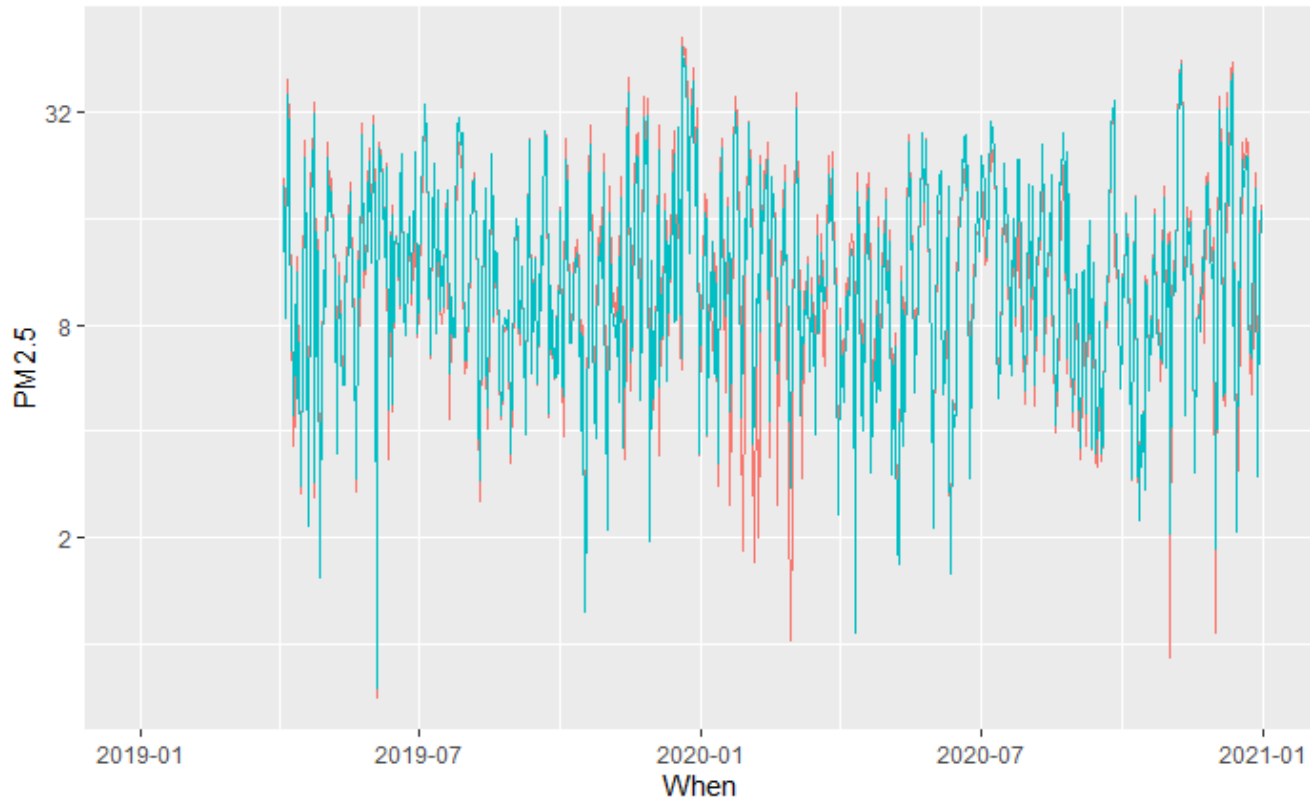


Other?

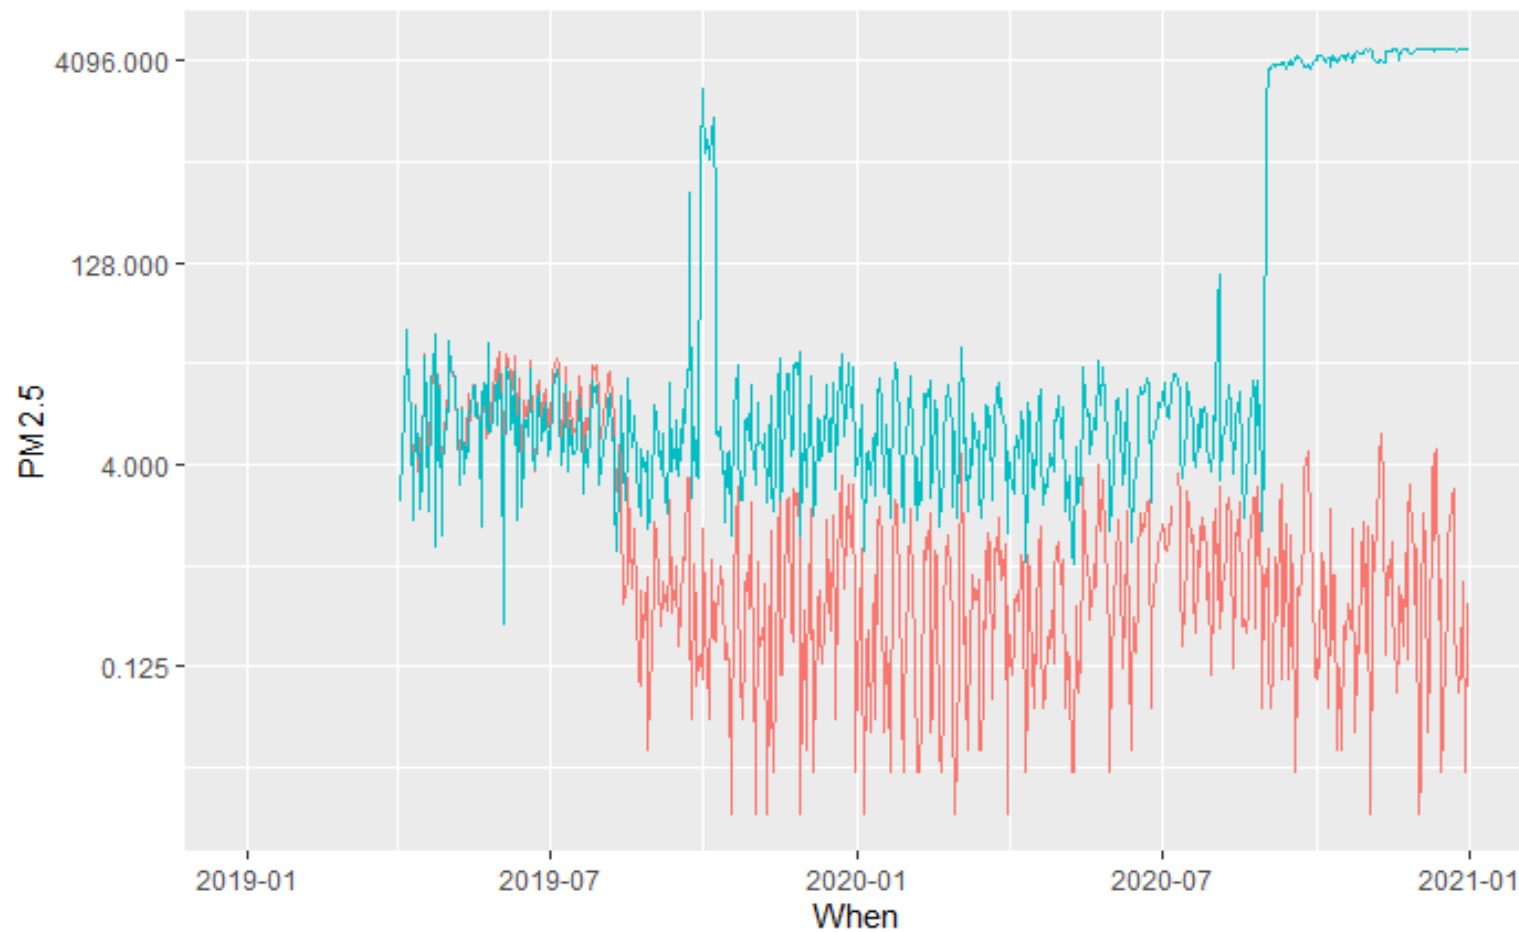

What can we learn? – July 2019

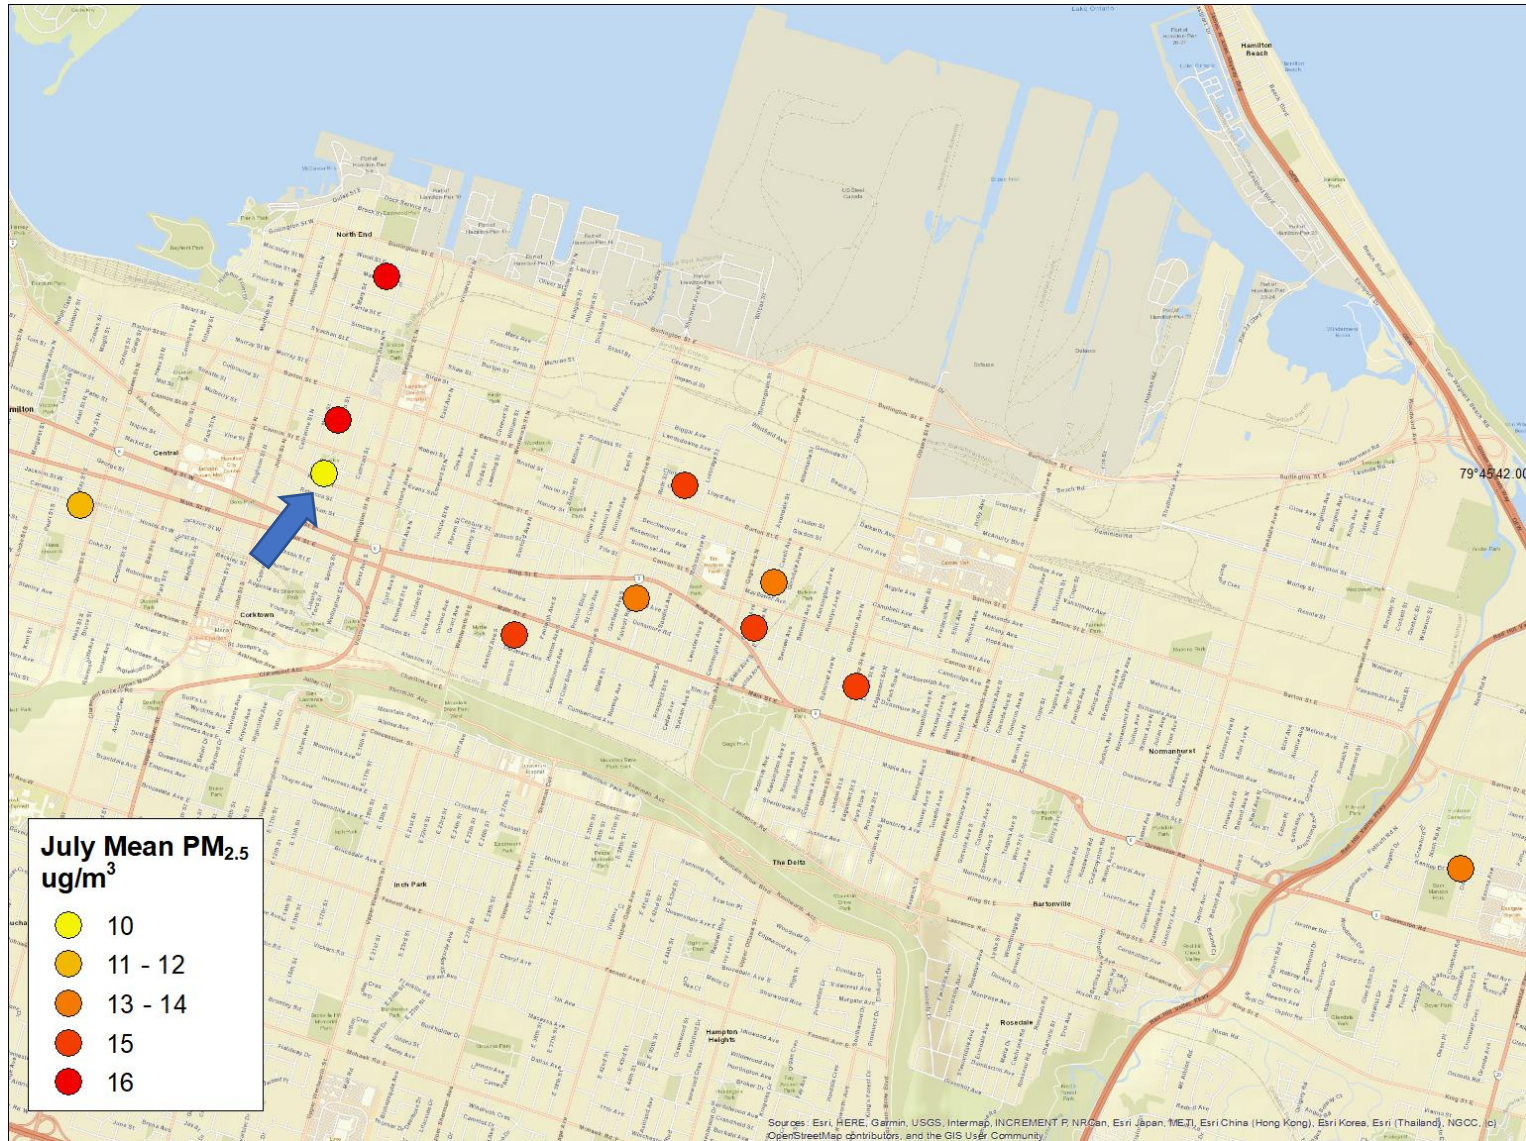

Uncorrected PurpleAir Daily Averages

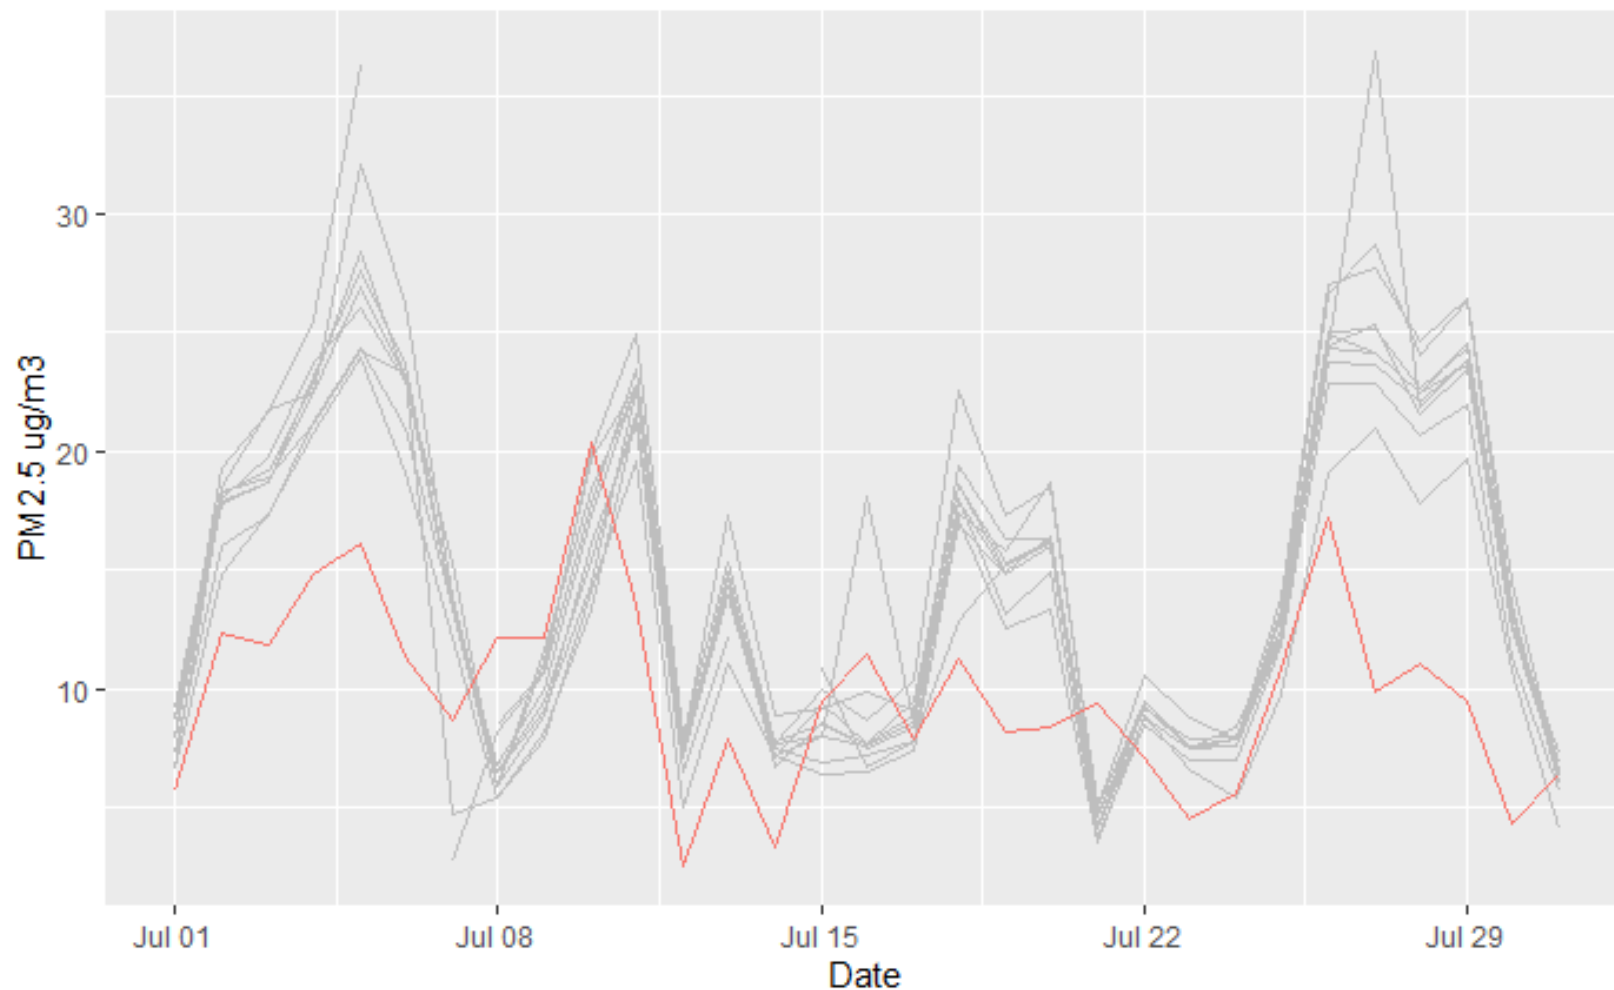

Conversions help accommodate different types of pollution with different particle densities.

For the same reason that wood floats and rocks sink in water, different particles have different densities - for example wild fire smoke vs road dust in the air. This is why a conversion may be needed when calculating the mass of any combination of particulates derived from particle counts.

None: No conversion applied to the data

US EPA: Courtesy of the United States Environmental Protection Agency Office of Research and Development, correction equation from their [US wide study](#) validated for wildfire and woodsmoke.

0-250 ug/m³ range (>250 may underestimate true PM_{2.5}):

$$PM_{2.5} (\mu g/m^3) = 0.534 \times PA(cf_1) - 0.0844 \times RH + 5.604$$

AQandU: Courtesy of the University of Utah, conversion factors from their [study of the PA sensors](#) during winter in Salt Lake City. [Visit their web site.](#)

$$PM_{2.5} (\mu g/m^3) = 0.778 \times PA + 2.65$$

LRAPA: Courtesy of the Lane Regional Air Protection Agency, conversion factors from their [study of the PA sensors](#). [Visit their web site.](#)

0 - 65 ug/m³ range:

$$LRAPA PM_{2.5} (\mu g/m^3) = 0.5 \times PA (PM_{2.5} CF=ATM) - 0.66$$

WOODSMOKE: From a study in Australia comparing Purple Air with NSW Government TEOM PM_{2.5} and Armidale Regional Council's DustTrak measurements - see published peer-reviewed study -

<https://www.mdpi.com/2073-4433/11/8/856/html>.

$$Woodsmoke PM_{2.5} (\mu g/m^3) = 0.5 \times PA (PM_{2.5} CF=ATM) - 0.66$$

Map Data Layer: ?

Conversion: ?



US EPA PM_{2.5} AQI

None

Standard

10 Minute Average



Outside
Sensors



Inside
Sensors



Show My
Sensors



Averages
as Rings

June 8th, 2021, 10:10:19 AM EDT

Why do we need to adjust PA data?


- Hygroscopic Growth




Air pollution monitors heat the incoming sample to address this issue. PA monitors do not.

Local Pollutant Conditions

- Particulate Matter is a mix of materials
- PA Sensors rely on light scattering as particles pass through a laser beam to infer mass from size
- Materials can vary in density (mass by volume)

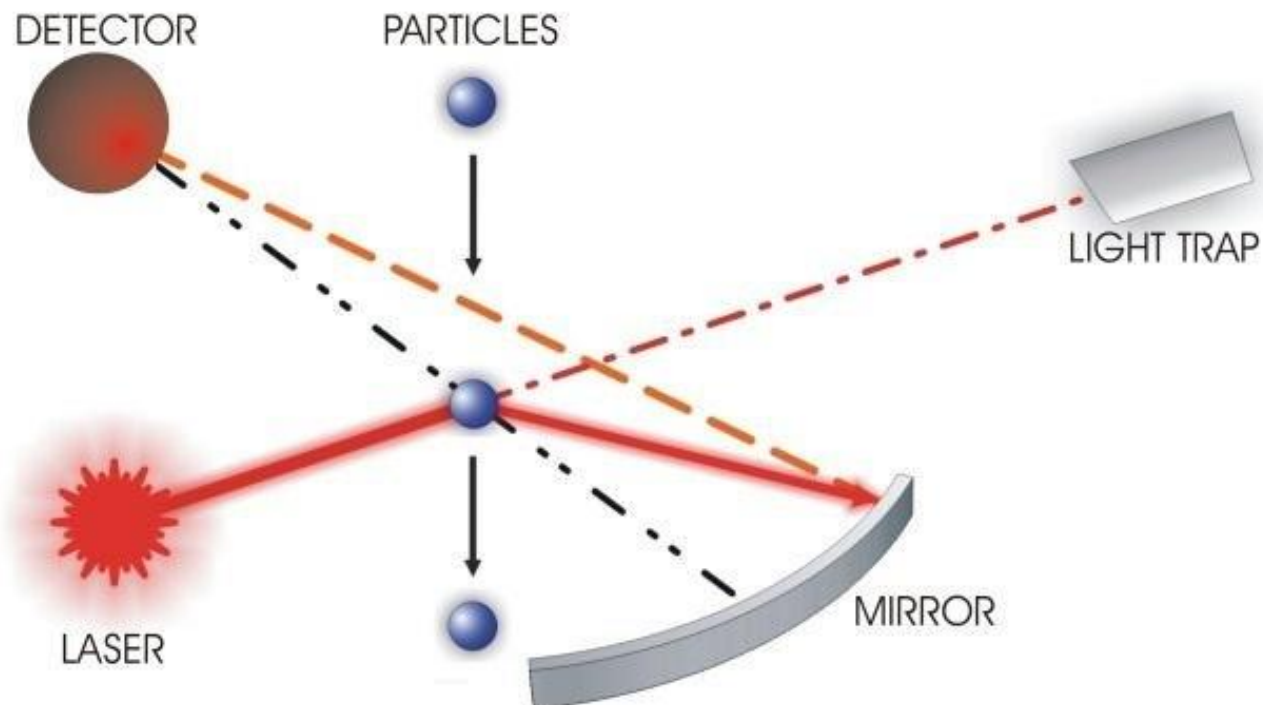

Corrected PurpleAir Daily Averages

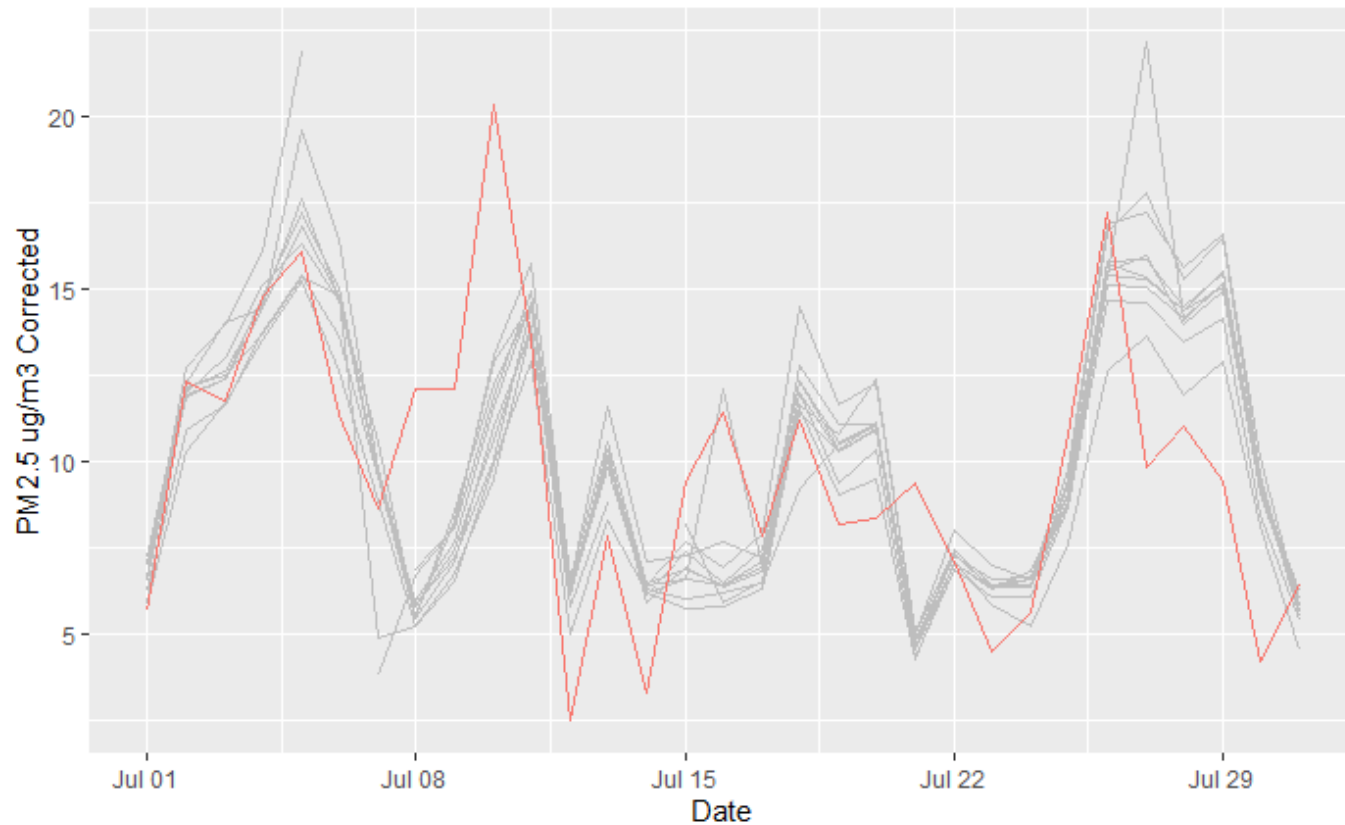

Initial Conclusions

- PA Sensors on their own will overestimate concentrations ~50-60%
- Corrected data provide little in terms of “new” information about spatial patterns of air pollution at a daily or monthly scale



Initial Conclusions

- Individual Monitors may systematically over or under predict concentrations
 - An individual would not know without collocation
 - Most likely over predict
- Short-term spikes in PA sensors may or may not be an artifact
 - Natural variations within an hour

Best Practices for Air Sensors

- Collocation of sensors with an Air Pollution Monitor
 - Establish local correction factor or validate existing correction factor
- Prefer sensors that measure 2x
- Repeat Collocation often
- Locate sensors at Air Pollution Monitor for length of study
- Life-span expectation: 1 year.